


# ELISA guide

Everything you need to perform  
your ELISA experiments

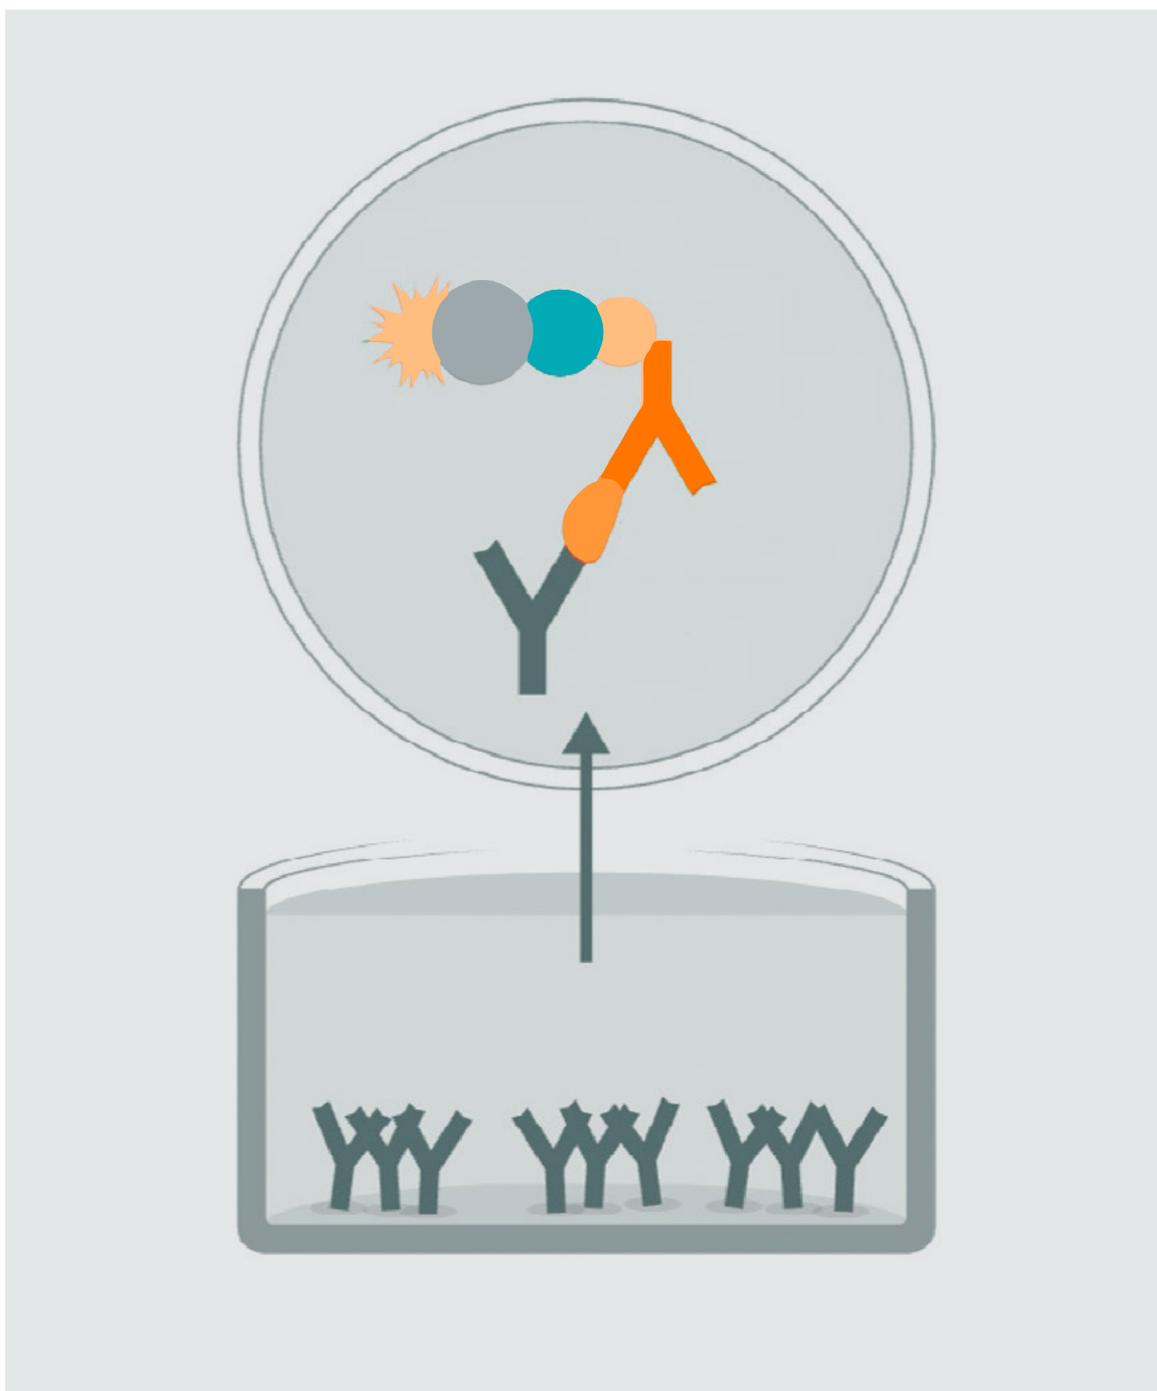

# Contents


<b>ELISA principle</b> .....	4
- Advantages and disadvantages of ELISA .....	5
<b>Types of ELISA</b> .....	6
- Direct ELISA .....	6
- Indirect ELISA .....	6
- Sandwich ELISA .....	7
-     SimpleStep ELISA® Kits .....	7
- Competitive ELISA .....	7
- Advantages and disadvantages of the different types of ELISA .....	8
<b>SimpleStep ELISA® kits</b> .....	9
- One-wash 90 minute protocols .....	9
- Uncompromising on sensitivity .....	10
- Tested in biological samples .....	10
- Wide range of analytes .....	11
- CatchPoint® SimpleStep ELISA® kits .....	11
<b>Matched antibody pair kits</b> .....	11
<b>Choose the right ELISA kit</b> .....	12
- ELISA sensitivity .....	12
- ELISA dynamic range .....	12
- ELISA CV .....	13
- ELISA specificity .....	13
- ELISA percent recovery .....	13
- ELISA linearity of dilution .....	13
<b>ELISA sample preparation guide</b> .....	14
- Tips for preparing your sample before running an ELISA .....	14
- Sample preparation methods .....	14
-     Cell culture supernatant .....	14
-     Cell extract .....	14
-     Conditioned medium .....	14
-     Milk .....	14
-     Plasma .....	14
-     Urine .....	15
-     Saliva .....	15
-     Serum .....	15
-     Tissue extract .....	15
- General recommendations .....	16

<b>Control samples required for ELISA</b> .....	16
- Positive control .....	16
- Negative control.....	16
- Standard.....	17
- Standard in sample matrix (spike control) control.....	17
- Endogenous positive control .....	17
<b>Sandwich ELISA protocol</b> .....	18
- Introduction .....	18
- Coating with capture antibody.....	19
- Blocking and adding samples .....	19
- Incubation with detection and secondary antibody.....	19
- Detection.....	20
- Data analysis.....	20
<b>ELISA analysis</b> .....	21
- ELISA standard curve .....	21
<b>Calculating and evaluating ELISA data</b> .....	22
- Calculating results .....	22
- Calculating the coefficient of variation .....	23
- Spike recovery .....	24
<b>ELISA troubleshooting tips</b> .....	25
- Poor standard curve .....	25
- No signal .....	25
- Large coefficient of variation (CV).....	26
- High background.....	27
- Low sensitivity.....	28
- Matrix effect.....	28

# ELISA principle

ELISA stands for enzyme-linked immunosorbent assay, also often referred to as enzyme immunoassay (EIA). An ELISA, like other types of immunoassays, relies on antibodies to detect a target antigen using highly specific antibody-antigen interactions. In an ELISA assay, the antigen must be immobilized to a solid surface. This is done either directly or via the use of a capture antibody itself immobilized on the surface. The antigen is then complexed to a detection antibody conjugated with a molecule amenable for detection such as an enzyme or a fluorophore.

An ELISA assay is typically performed in a multi-well plate (96- or 384-wells). The multi-well plate provides the solid surface to immobilize the antigen. Immobilization of the analytes facilitates separation of the antigen from the rest of the components in the sample. This characteristic makes ELISA one of the easiest assays to perform on multiple samples simultaneously.

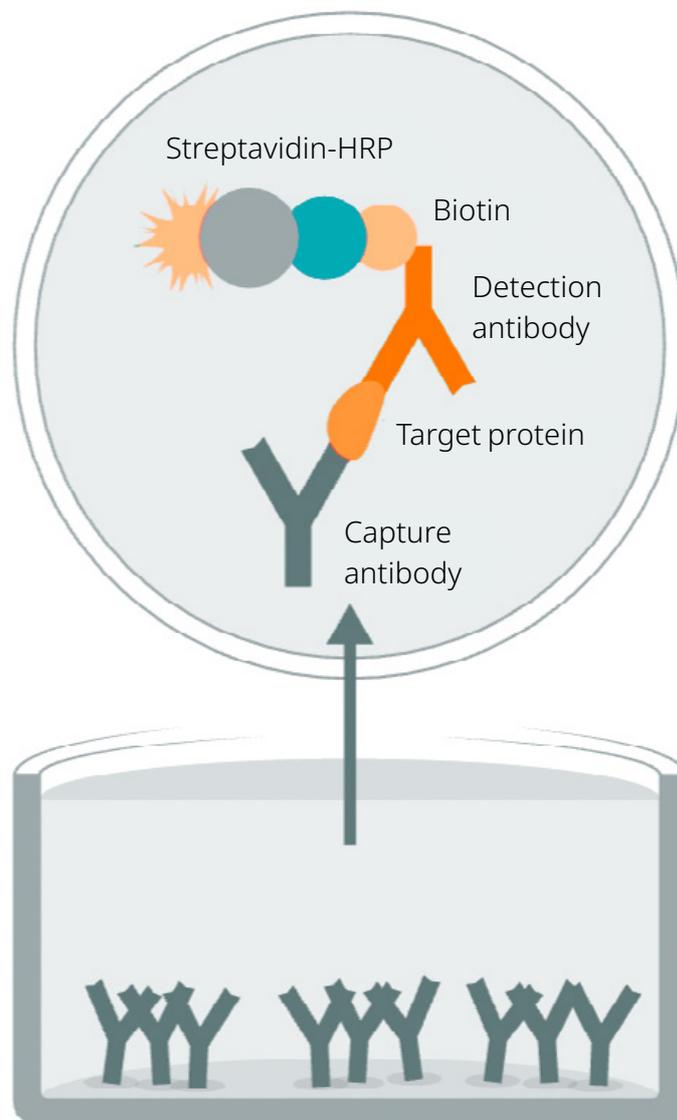

## Advantages and disadvantages of ELISA

### Advantages

High sensitivity and specificity: it is common for ELISAs to detect antigens at the picogram level in a very specific manner due to the use of antibodies.

High throughput: commercial ELISA kits are normally available in a 96-well plate format. But the assay can be easily adapted to 384-well plates.

Easy to perform: protocols are easy to follow and involve little hands-on time.

Quantitative: it can determine the concentration of antigen in a sample.

Possibility to test various sample types: serum, plasma, cellular and tissue extracts, urine, and saliva among others.

### Disadvantages

Temporary readouts: detection is based on enzyme/substrate reactions and therefore readout must be obtained in a short time span.

Limited antigen information: information limited to amount or presence of the antigen in the sample.

These are the general ELISA advantages and disadvantages. There are other advantages and disadvantages depending on the type of ELISA used as explained in the next section.

# Types of ELISA

ELISA assays can be found in different formats, each one with its own advantages and disadvantages. The diagram below illustrates the four main different types of ELISA.



## Direct ELISA

The antigen is immobilized to the surface of the multi-well plate and detected with an antibody specific for the antigen and directly conjugated to HRP or other detection molecules.

## Indirect ELISA

Similar to direct ELISA assays, the antigen is immobilized to the surface of the multi-well plate. However, a two-step process is required for detection whereby a primary antibody specific for the antigen binds to the target, and a labeled secondary antibody against the host species of the primary antibody binds to the primary antibody for detection.

The method can also be used to detect specific antibodies in a serum sample by substituting the serum for the primary antibody.

See all indirect ELISA kits at [www.abcam.com/indirect-ELISA-kits](http://www.abcam.com/indirect-ELISA-kits)

## **Sandwich ELISA**

Sandwich ELISA (or sandwich immunoassay) is the most commonly used format. This format requires two antibodies specific for different epitopes of the antigen. These two antibodies are normally referred to as matched antibody pairs. One of the antibodies is coated on the surface of the multi-well plate and used as a capture antibody to facilitate the immobilization of the antigen. The other antibody is conjugated and facilitates the detection of the antigen.

See all sandwich ELISA kits at [www.abcam.com/sandwich-ELISA-kits](http://www.abcam.com/sandwich-ELISA-kits)

## **SimpleStep ELISA® Kits**

Our SimpleStep ELISA® kits provides improved speed and performance while retaining the familiar process and standard data output of a traditional ELISA kit. SimpleStep ELISA® kits reduce the number of wash steps by enabling the sandwich complex formation in one step rather than sequentially. Total time required is less than two hours.

See all SimpleStep ELISA® kits at [www.abcam.com/simplestep-ELISA-kits](http://www.abcam.com/simplestep-ELISA-kits)

## **Competitive ELISA**

Also known as inhibition ELISA or competitive immunoassay, this assay measures the concentration of an antigen by detection of signal interference. Each of the previous formats can be adapted to the competitive format. The sample antigen competes with a reference antigen for binding to a specific amount of labeled antibody. The reference antigen is pre-coated on a multi-well plate. The sample is pre-incubated with labeled antibody and added to the wells. Depending on the amount of antigen in the sample, more or less free antibodies will be available to bind the reference antigen. This means the more antigen there is in the sample, the less reference antigen will be detected and the weaker the signal.

Some competitive ELISA kits use labeled antigen instead of labeled antibody. The labeled antigen and the sample antigen (unlabeled) compete for binding to the primary antibody. The lower the amount of antigen in the sample, the stronger the signal due to more labelled antigen in the well.

See all competitive ELISA kits at [www.abcam.com/competitive-ELISA-kits](http://www.abcam.com/competitive-ELISA-kits)

## Advantages and disadvantages of the different types of ELISA

	<b>Advantages</b>	<b>Disadvantages</b>
Direct ELISA	<p>Short protocol: saves time and reagents.</p> <p>No cross-reactivity from secondary antibody.</p>	<p>Potential high background: all proteins in the sample bind to the surface.</p> <p>No signal amplification.</p> <p>Low flexibility: the primary antibody must be conjugated.</p>
Indirect ELISA	<p>Signal amplification: several secondary antibodies will bind to the primary antibody.</p> <p>High flexibility: the same secondary antibody may be used for several primary antibodies.</p>	<p>Long protocol if compared to direct ELISA.</p> <p>Potential cross-reactivity from secondary antibody.</p>
Sandwich ELISA	<p>High specificity: involves two antibodies detecting different epitopes on the same antigen.</p> <p>Suitable for complex samples.</p> <p>High flexibility and sensitivity: both direct and indirect methods can be used.</p>	<p>Demanding design: finding two antibodies against the same target that recognize different epitopes and work well together can be challenging at times.</p>
Competitive ELISA	<p>Depends on base ELISA selected.</p> <p>Suitable for small antigens.</p>	<p>Depends on base ELISA selected.</p>

# SimpleStep ELISA® kits

Save time without compromising on performance. Upgrade your ELISA for specific and sensitive results with a single-wash protocol.


- Single-wash protocol reduces assay time to 90 minutes or less
- Comparable or better sensitivity than competitor assays
- Fully validated in biological samples
- No special equipment required

## Your ELISA upgrade:

	Conventional ELISA kits	SimpleStep ELISA® kits	
Sensitivity	✓✓	✓✓✓✓	Liquid-phase reaction system drives higher sensitivity
Reproducibility	✓✓	✓✓✓✓	Recombinant antibodies provide better reproducibility
Full validation	✓	✓✓✓✓	Validation on biological samples ensures reaction with endogenous protein
Fast and easy protocol		✓✓✓✓	One-wash 90-minute protocol for fewer handling steps

## One-wash 90-minute protocol

With SimpleStep ELISA® kits, an analyte-capture and detector antibody sandwich complex is formed in solution. In just one incubation and wash step, the complete sandwich complex forms in the well and is anchored to the plate with an immunoaffinity tag.

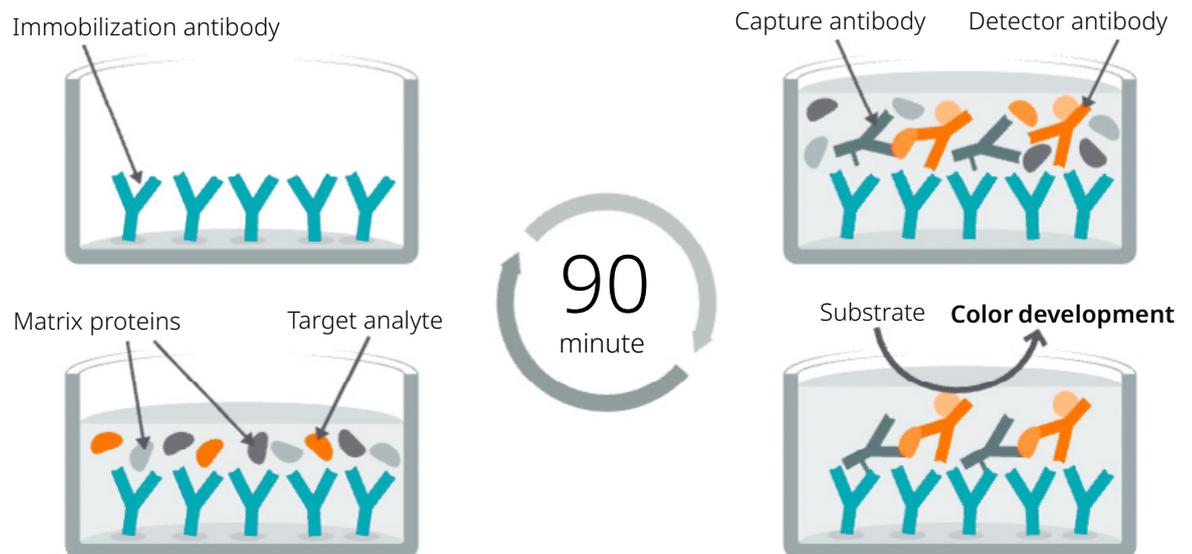


See the video of how SimpleStep ELISA® works at [www.abcam.com/simplestep-elisa-video](http://www.abcam.com/simplestep-elisa-video)

## Uncompromising on sensitivity

SimpleStep ELISA® kits drastically reduce assay times without compromising on performance. We compared the sensitivity of SimpleStep ELISA® kits to the most popular competitor brand of ELISA kits for 75 popular human and mouse proteins. SimpleStep ELISA® kits show superior sensitivity in 56 out of 75 cases.

### Sensitivity: SimpleStep ELISA® vs competitor

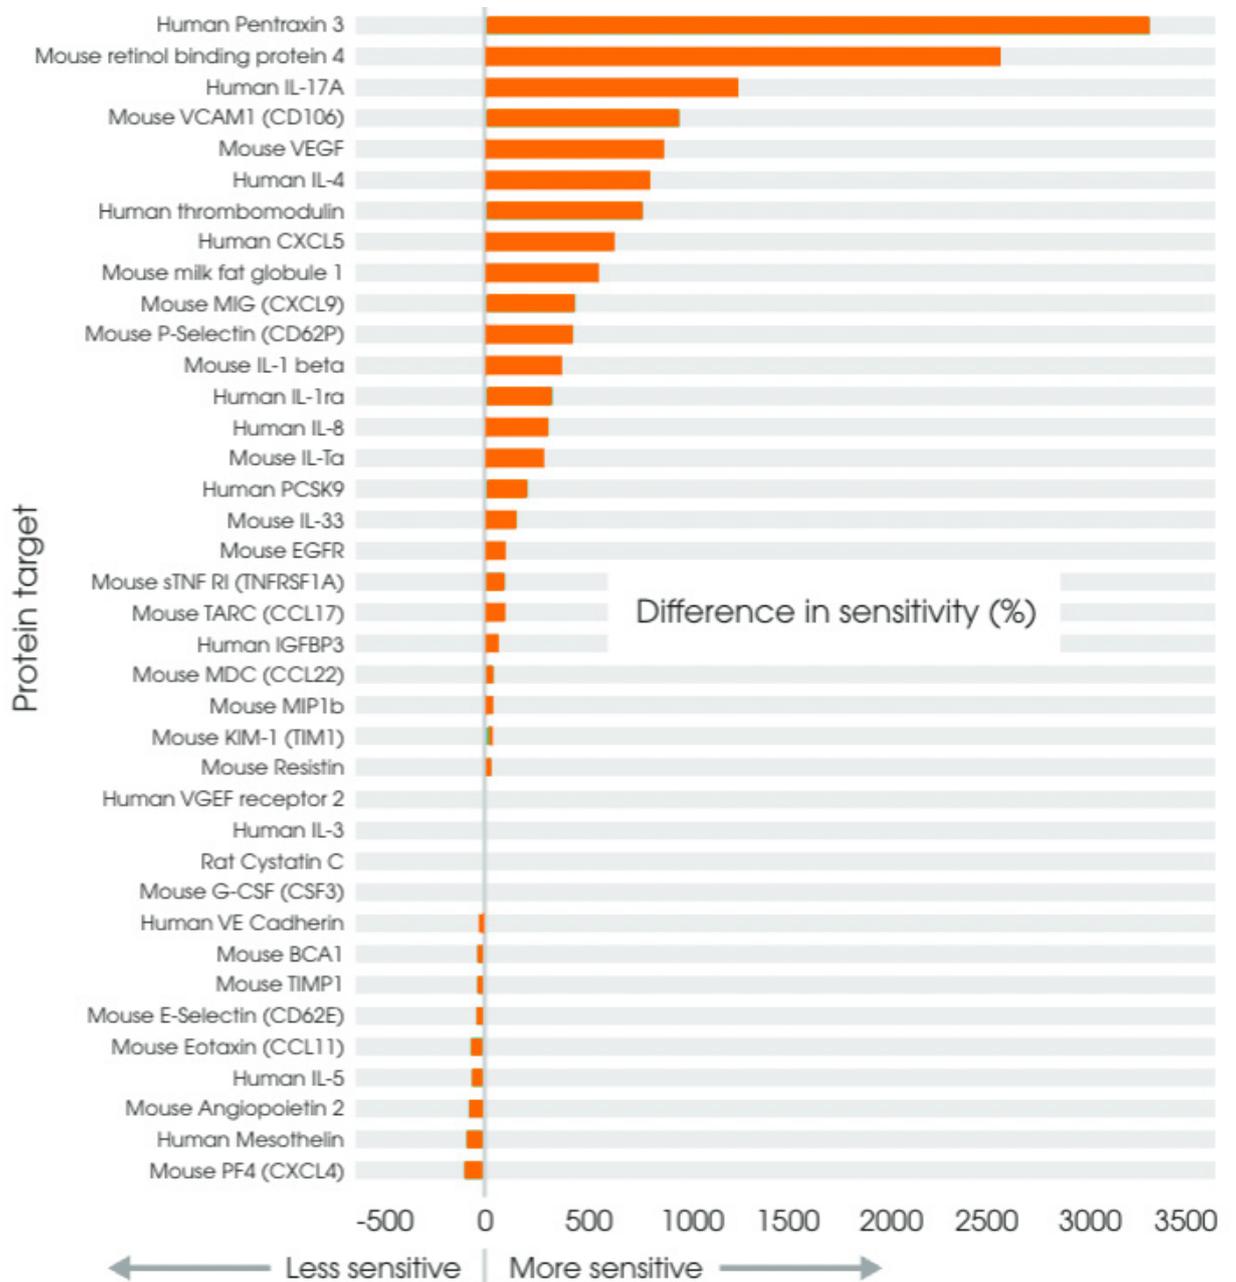

## Tested in biological samples

Every SimpleStep ELISA® kit is validated using multiple biological samples for assay specificity. All secreted serum or plasma-based targets are tested and fall within World Health Organization blood reference ranges. When available, the SimpleStep ELISA® kits are calibrated against known NIBSC international standards and includes a conversion factor for data comparison.

## Wide range of analytes

We currently have SimpleStep ELISA® kits to almost 600 targets, including popular proteins like PD-L1, GFP, and fibrinogen, and are continually adding more to the catalog.

See all SimpleStep ELISA® kits at [www.abcam.com/simplestep-ELISA-kits](http://www.abcam.com/simplestep-ELISA-kits)

## CatchPoint® SimpleStep ELISA® kits

CatchPoint SimpleStep ELISA® kits have been developed using a fluorescent substrate to provide improved linearity over an extended dynamic range when compared to colorimetric ELISA kits. The extended dynamic range provides better quantification at both the lower and the upper end of the curve.

Find out more at [www.abcam.com/catchpoint-simplestep-elisa-kits](http://www.abcam.com/catchpoint-simplestep-elisa-kits)


## Matched antibody pair kits

Create your own ELISA with high-performing antibody pairs.

Matched antibody pair kits and reagents deliver consistent, specific, and sensitive results.

- Batch-to-batch consistency: only recombinant monoclonal antibodies are used in our matched antibody pairs.
- Specificity: antibody pairs are screened in plasma and serum to ensure specificity in complex samples.
- Sensitivity: benchmarked against commercially available antibody pairs to ensure equivalent or superior performance compared with the competition.

Matched antibody pair kits include a titrated capture and biotinylated detector antibody pair and a calibrated protein standard. Kits are available in two sizes, with enough reagents for either 2 or 10 x 96-well plates using a standard sandwich ELISA.

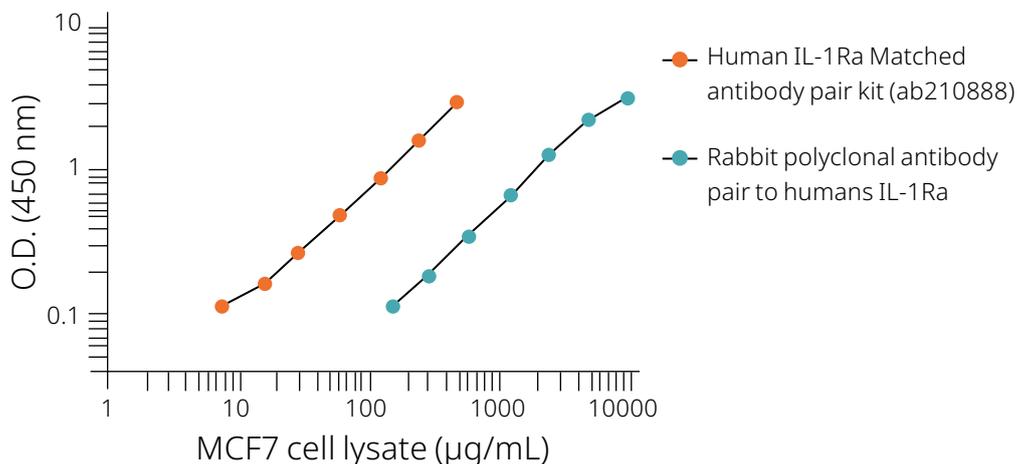

The human IL-1Ra matched antibody pair kit (ab210888) is 10-fold more sensitive than a rabbit polyclonal antibody pair when measuring human IL-1Ra standard protein using a sandwich ELISA.

See all our matched antibody pairs at [www.abcam.com/matched-antibody-pairs](http://www.abcam.com/matched-antibody-pairs)

# Choose the right ELISA kit

Careful evaluation of assay performance is an important first step in choosing a new ELISA kit. Important parameters include sensitivity, dynamic range and precision, which are reported for most ELISA kits. Other parameters are more predictive of ELISA performance for typical sample types. Percent (%) recovery and linearity of dilution measure the target protein in real samples, such as plasma, serum or cell culture media.

This chapter explains how to interpret the different parameters to help you find the right ELISA kit for your sample.

Summary of parameters to look for when choosing an ELISA kit:

<b>Parameter</b>	<b>Acceptance criteria</b>
Sensitivity	Depends on the target protein*
Dynamic range	
CV (%) for intra-assay precision	≤ 10%
CV (%) for inter-assay precision	≤ 15%
Specificity	Check reactivity with highly homologous proteins
% Recovery	≥ 80%
Linearity of dilution	≤ 20% difference from undiluted sample

## ELISA sensitivity

Sensitivity is the lowest level of protein that the antibody pair used in the ELISA kit can detect.

## ELISA dynamic range

The dynamic range is defined as the upper and lower concentrations of the target protein that the assay can accurately quantify.

\*It is important to know what levels of the target protein are expected in a sample to check that the sensitivity and dynamic range of a given ELISA kit are appropriate. Samples with high concentrations of the target protein can be diluted so that the raw signal falls within the dynamic range of the assay.

Reported values for those two parameters can be misleading because they are often determined by using standard protein in simple buffers. This may not reflect the kinetic of detection of an endogenous protein in a biological sample.

## **ELISA CV**

The CV (%) or coefficient of variability shows how consistent the assay is.

CV is generally calculated to evaluate the inter-assay precision or plate-to-plate consistency and the intra-assay precision or consistency between duplicates run in the same experiment.

- Inter-assay % CVs of less than 15 are generally acceptable.
- Intra-assay % CVs should be less than 10.

## **ELISA specificity**

It is important that the antibodies used in the ELISA kit do not cross-react with non-target proteins. These can be proteins of high homology across species.

For instance, Human Factor IX SimpleStep ELISA® Kit (ab188393), is specific of human Factor IX and does not react with mouse, rat, rabbit, goat, guinea pig, hamster, cow, dog or pig sample.

## **ELISA percent recovery**

Percent (%) recovery is determined by spiking a known amount of purified target protein into a biological sample type (also called sample matrix). For secreted proteins such as cytokines, typical sample matrices are plasma and serum; for intracellular proteins such as kinases, samples are cell culture lysates.

The spiked sample is measured in the ELISA, and the concentration is calculated from the standard curve. This calculated concentration is compared to the known concentration of the protein and is expressed as a percentage. For example, 100% recovery means that the observed concentration was the same as the actual concentration of spiked protein in the sample. It suggests that other proteins and molecules in the sample type did not interfere in the quantification of the target protein.

If % recovery measures less than 80% for a specific sample type, then a different ELISA kit should be selected for quantification.

## **ELISA linearity of dilution**

Linearity of dilution is a good companion to % recovery because it measures native rather than spiked protein in biological samples. Linearity of dilution is determined by measuring multiple dilutions of known positive samples by ELISA. The concentration of the target protein is determined by multiplying the dilution factor by the calculated concentration. For best results, the concentration of the samples should be similar for all dilutions. If a difference of more than 20% from the undiluted sample is observed, then a different ELISA kit should be chosen for accurate quantification.

# ELISA sample preparation

## Tips for preparing your sample before running an ELISA

Please refer to the protocol included with your kit for product-specific details regarding sample preparation and compatible sample types.

These guidelines are intended to be an educational resource for preparing commonly tested samples for use in ELISA assays. Optimum sample preparation procedures will vary depending on the target and assay of interest. It is always good practice to consult the literature for experimental examples similar to your own when developing a new assay.

## Sample preparation methods

### Cell culture supernatant

- Pipette cell culture media into a centrifuge tube and centrifuge at 1,500 rpm for 10 min at 4°C.
- Immediately aliquot supernatant and store samples at -80°C. Minimize freeze/thaw cycles.

### Cell extract

- Place tissue culture plates on ice.
- Aspirate medium and gently wash cells once with ice-cold PBS.
- Aspirate PBS and add 0.5 mL complete extraction buffer per 100 mm plate.
- Scrape cells to collect in tilted plate and remove to pre-chilled tube.
- Vortex briefly and incubate on ice for 15–30 min.
- Centrifuge at 13,000 rpm for 10 min at 4°C to pellet insoluble contents.
- Aliquot supernatant (this is the soluble cell extract) to clean, chilled tubes on ice and store samples at -80°C. Minimize freeze/thaw cycles.

### Conditioned medium

- Place cells in complete (serum-containing) growth medium and allow cells to proliferate to desired level of confluence.
- Remove growth medium and wash very gently with a few mL of warm PBS. Repeat wash step.
- Remove last PBS wash and gently add serum free growth medium.
- Incubate 1–2 days.
- Pipette medium into a centrifuge tube and centrifuge at 1,500 rpm for 10 min at 4°C.
- Immediately aliquot supernatant and store samples at -80°C. Minimize freeze/thaw cycles.

### Milk

- Collect samples and centrifuge at 10,000 x g for 2 min at 4°C.
- Aliquot supernatant and store samples at -80°C. Minimize freeze/thaw cycles.

### Plasma

- Collect whole blood into anti-coagulant containing tube or add 0.1 M sodium citrate to 1/10 final volume.
- Centrifuge at 3,000 rpm for 10 min at 4°C.
- Immediately aliquot supernatant (plasma) and store samples at -80°C. Minimize freeze/thaw cycles.

### **Urine**

- Collect samples and centrifuge at 10,000 x g for 2 min at 4°C.
- Aliquot supernatant and store samples at -80°C. Minimize freeze/thaw cycles.

### **Saliva**

- Collect samples and centrifuge at 10,000 x g for 2 min at 4°C.
- Aliquot supernatant and store samples at -80°C. Minimize freeze/thaw cycles.

### **Serum**

- Collect whole blood in untreated test tube or, for example, an anti-coagulant free tube.
- Incubate undisturbed at room temperature for 20 min.
- Centrifuge at 3,000 rpm for 10 min at 4°C.
- Immediately aliquot supernatant (serum) and store samples at -80°C. Minimize freeze/thaw cycles.

### **Tissue extract**

- Dissect the tissue of interest with clean tools, preferably on ice and as quickly as possible to prevent degradation by proteases.
- Place the tissue in round bottom microfuge tubes and immerse in liquid nitrogen to snap freeze. Store samples at -80°C for later use or keep on ice for immediate homogenization.
- For a ~5 mg piece of tissue, add ~300 µL complete extraction buffer (see cell/tissue extraction buffer recipe) to the tube and homogenize with an electric homogenizer.
- Rinse the blade twice using 300 µL complete extraction buffer for each rinse, then maintain constant agitation for 2 h at 4°C (eg place on an orbital shaker in the cold room).
- Centrifuge for 20 min at 13,000 rpm at 4°C. Place on ice, aliquot supernatant (this is the soluble protein extract) to a fresh, chilled tube and store samples at -80°C. Minimize freeze/thaw cycles

**Volumes of lysis buffer must be determined in relation to the amount of tissue present.  
Typical concentration of final protein extract is >1 mg/mL.**

### **Cell/tissue extraction buffer recipe**

- 100 mM Tris, pH 7.4
- 150 mM NaCl
- 1 mM EGTA
- 1 mM EDTA
- 1% Triton X-100
- 0.5% Sodium deoxycholate

Additional reagents required to produce complete extraction buffer.

- Phosphatase inhibitor cocktail
- Protease inhibitor cocktail
- PMSF

**Supplement the cell extraction buffer with phosphatase and protease inhibitor cocktails as described by manufacturer, and PMSF to 1 mM, immediately before use.**

## General recommendations

- Recommended protein extract concentration is at least 1–2 mg/mL.
- Typically, serum, plasma, cell and tissue extracts are diluted by 50% with binding buffer.
- Prior to use after thawing, centrifuge samples at 10,000 rpm for 5 minutes at 4°C to remove any precipitate.

# Control samples required for ELISA

Running the appropriate controls helps you to accurately separate true positive results from potentially false results. Positive and negative controls will also be useful if you ever need to troubleshoot your protocol. Here we explain the various types of control samples you should use when running an ELISA.

## Positive control

Use either an endogenous soluble sample known to contain the protein you are detecting or a purified protein or peptide known to contain the immunogen sequence for the antibody you are using. A positive result from the positive control, even if the samples are negative, will indicate the procedure is optimized and working. It will verify that any negative results are valid.

We recommend checking the antibody datasheet, which will often provide a suggested positive control. If no control is suggested, we recommend the following:


- Check to see if there are any Abreviews® for the antibody. Any tissues, cells, or lysates that have been used successfully can be considered a suitable positive control.
- Try looking at the Swiss-Prot or Omnigene database links on the datasheet. These databases will often have a list of tissues that the protein is expressed in. These can also be considered suitable positive controls.
- Check the GeneCards entry for the protein. This will usually provide you with relative levels of expression in various tissues.
- If you still have difficulty finding a suitable control, we recommend doing a quick literature search on PubMed to see which tissues and cells express the protein of interest.

## Negative control

This is a sample that does not express the protein you are detecting, which allows you to check for non-specific binding and false positive results. Each plate you use should contain a negative control sample to validate the results.

## Standard

This is a sample that contains a known concentration of the target protein, from which the standard curve can be obtained. For example, below is a typical standard curve from our Mouse IL-6 ELISA kit (ab46100) with concentration ranging from 15.6 to 500 pg/mL. A poor standard curve means the antibody didn't bind properly or doesn't capture the protein standard. The R2 value of the trend line should be >0.99.

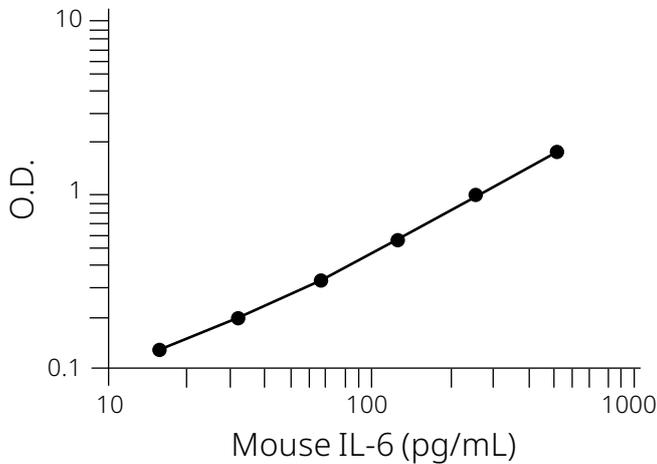

## Standard in sample matrix (spike control) control

When testing serum samples in ELISA, include a standard in normal diluent buffer as usual. But we recommend to also include a standard diluted in serum from the species you are testing. The two can then be compared to ensure there is no effect on the standard curve from other proteins in the serum. This is known as a spike control and tells you that a target protein is recoverable after being spiked into a matrix. Acceptable results are 80–120%.

## Endogenous positive control

We recommend including an endogenous positive control if you are testing a recombinant protein sample. This should be an essential component of your experiment.

There are inherent difficulties with antibody detection of recombinant proteins that need to be considered. Folding of the recombinant protein may be different from the endogenous native form and may prevent antibody access to the epitope. This is particularly the case with tagged proteins. Always ensure tags are placed on the N or C-terminal end of the recombinant protein.

Most importantly, always ensure the recombinant protein includes the immunogen sequence of the antibody you are using. An endogenous positive control is important to validate the results, as well as to indicate how well the reagents (eg antibodies) and procedure are working.


# Sandwich ELISA protocol

## Introduction

A sandwich ELISA measures antigen between two layers of antibodies (capture and detection antibody). The target antigen must contain at least two antigenic sites capable of binding to antibodies.

Monoclonal or polyclonal antibodies can be used as the capture and detection antibodies in sandwich ELISA systems. Monoclonal antibodies recognize a single epitope that allows quantification of small differences in antigen. A polyclonal is often used as the capture antibody to pull down as much of the antigen as possible.

Sandwich ELISAs remove the sample purification step before analysis and enhance sensitivity (2–5 times more sensitive than direct or indirect).

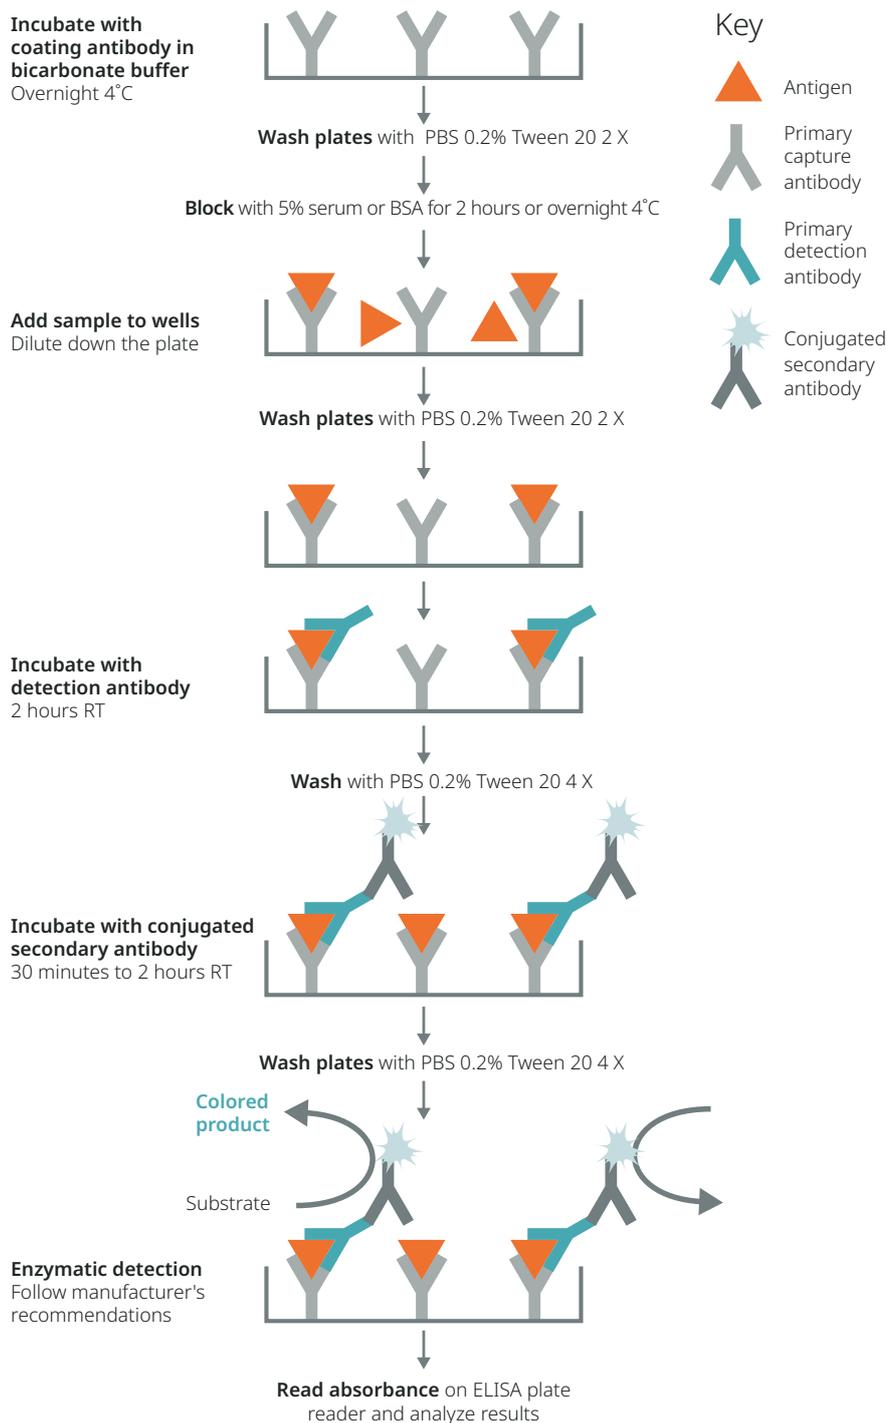

Sandwich ELISA procedures can be difficult to optimize, and tested matched antibody pairs should be used. This ensures the antibodies are detecting different epitopes on the target protein and do not interfere with the other antibody binding. We are unable to guarantee the performance of our antibodies in sandwich ELISA unless they have been specifically tested.

Always review antibody datasheets for tested applications information.

## Coating with capture antibody

1. Coat the wells of a PVC microtiter plate with the capture antibody at 1–10 µg/mL concentration in carbonate/bicarbonate buffer (pH 9.6).

*Unpurified antibodies (eg ascites fluid or antiserum) may require increased concentration of the sample protein (try 10 µg/mL) to compensate for the lower concentration of specific antibody.*

2. Cover the plate with adhesive plastic and incubate overnight at 4°C.
3. Remove the coating solution and wash the plate twice by filling the wells with 200 µL PBS. The solutions or washes are removed by flicking the plate over a sink. The remaining drops are removed by patting the plate on a paper towel.

## Blocking and adding samples

1. Block the remaining protein-binding sites in the coated wells by adding 200 µL blocking buffer (5% non-fat dry milk/PBS) per well.
2. Cover the plate with adhesive plastic and incubate for at least 1–2 h at room temperature or overnight at 4°C.
3. Wash the plate twice with 200 µL PBS.
4. Add 100 µL of diluted samples to each well. Always compare signal of unknown samples against those of a standard curve. Run standards (duplicates or triplicates) and blank with each plate. Incubate for 90 min at 37°C.

*Ensure concentration of standards span the most dynamic detection range of antibody binding. You may need to optimize the concentration range to obtain a suitable standard curve. Always run samples and standards in duplicate or triplicate.*

5. Remove samples and wash the plate twice with 200 µL PBS.

## Incubation with detection and secondary antibody

1. Add 100 µL of diluted detection antibody to each well.

*Check that the detection antibody recognizes a different epitope on the target protein to the capture antibody. This prevents interference with antibody binding. Use a tested matched pair whenever possible.*

2. Cover the plate with adhesive plastic and incubate for 2 h at room temperature.
3. Wash the plate four times with PBS.
4. Add 100 µL of conjugated secondary antibody, diluted in blocking buffer immediately before use.
5. Cover the plate with adhesive plastic and incubate for 1–2 h at room temperature.
6. Wash the plate four times with PBS.

## Detection

Horse radish peroxidase (HRP) and alkaline phosphatase (ALP) are the two most widely used enzymes for detection in ELISA assays.

Consider that some biological materials have high levels of endogenous enzyme activity (such as high ALP in alveolar cells, high peroxidase in red blood cells) that may result in nonspecific signal. If necessary, perform an additional blocking treatment with levamisol (for ALP) or 0.3%  $\text{H}_2\text{O}_2$  in methanol (for peroxidase).

### ALP substrate

P-Nitrophenyl-phosphate (pNPP) is the most widely used substrate for most applications. Measure the yellow color of nitrophenol at 405 nm after 15–30 min incubation at room temperature and stop the reaction by adding equal volume of 0.75 M NaOH.

### HRP chromogenes

The substrate for HRP is hydrogen peroxide. Cleavage of hydrogen peroxide is coupled to oxidation of a hydrogen donor which changes color during reaction.

### TMB (3,3',5,5'-tetramethylbenzidine)

Add TMB solution to each well, incubate for 15–30 min, add equal volume of stopping solution (2 M  $\text{H}_2\text{SO}_4$ ) and read the optical density at 450 nm.

### OPD (o-phenylenediamine dihydrochloride)

The end product is measured at 492 nm. Keep and store the substrate in the dark as it is light sensitive.

### ABTS (2,2'-azino-di-[3-ethyl-benzothiazoline-6 sulfonic acid] diammonium salt)

The end product is green and the optical density can be measured at 416 nm.

Always handle with care and wear gloves as some enzyme substrates are considered hazardous (potential carcinogens).

## Data analysis

Prepare a standard curve from the serial dilutions data with concentration on the x axis (log scale) vs absorbance on the Y axis (linear). Interpolate the concentration of the sample from this standard curve.

# ELISA analysis

ELISA assays can be classified as follows according to the type of data obtained:


- **Qualitative ELISA:** only determines whether the antigen is present or not in the sample. It requires a blank well containing no antigen or an unrelated control antigen.
- **Semi-quantitative ELISA:** allows the relative comparison of the antigen levels between the samples.
- **Quantitative ELISA:** allows calculating the amount of antigen present in the sample. It requires comparison of the values measured for the samples with a standard curve prepared from a serial dilution of a purified antigen in a known concentration. This is the most commonly reported ELISA data.

## ELISA standard curve

The standard or calibration curve is the element of the quantitative ELISA that will allow calculating the concentration of antigen in the sample.

The standard curve is derived from plotting known concentrations of a reference antigen against the readout obtained for each concentration (usually optical density at 450 nm).

Most ELISA plate readers will incorporate a software for curve fitting and data analysis. The concentration of the antigen in the sample is calculated by extrapolation of the linear portion of the standard curve.

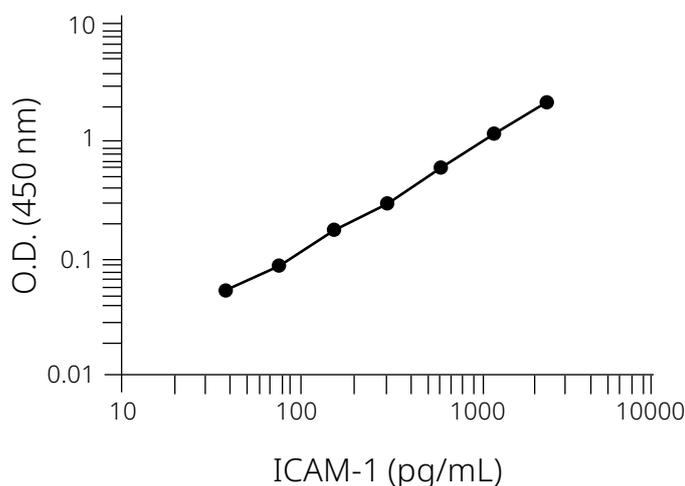

Example of a quantitative ELISA standard curve from Human ICAM1 SimpleStep ELISA® Kit (ab174445).

Curve fitting software allow using different models to plot your data.

- **Linear plot:** presents the concentration of the antigen in one axis and the readout in the other. R<sup>2</sup> values are normally used here to determine fitting, with values higher than 0.99 representing a very good fit. However, linear plots tend to compress data points on the lower end of the curve resulting in decreased resolution.
- **Semi-log plot:** helps counteracting the compression at the lower end caused by linear plots. Semi-log plots use the log of the concentration against the readout. This method commonly results in a sigmoidal curve that distributes more evenly the data points.
- **Log/log plot:** provides good linearity for the low to medium range of the concentrations. The higher end of the range tends to lose linearity.
- **4- or 5-parameter logistic (4PL or 5PL) curves:** they are more sophisticated methods that take into account other parameters such as maximum and minimum and therefore require more complex calculations. 4PL assumes symmetry around the inflection point while 5PL takes asymmetry into account, which normally is a better fit for immunoassays.

If your software allows it, 4-PL and 5-PL will fit most ELISA calibration standard curves. If not, the best option is to use a semi-log or a log/log plot.

# Calculating and evaluating ELISA data

Calculation of results from ELISA data and recommended guidelines on statistical assay validation.

## Calculating results

Always run ELISA samples in duplicate or triplicate. This will provide enough data for statistical validation of the results. Many computer programs are now available to help process ELISA results in this way.

Calculate the average absorbance values for each set of duplicate standards and duplicate samples. Duplicates should be within 20% of the mean.


### Standard curve

Create a standard curve for the target protein by plotting the mean absorbance (y axis) against the protein concentration (x axis). Draw the best fit curve through the points in the graph (we suggest using a suitable computer program for this).

We recommend including a standard on each ELISA plate to provide a standard curve for each plate used.

A representative standard curve is shown in the figure below, from human HIF1 alpha SimpleStep ELISA® kit (ab171577). Each point on the graph represents the mean of the three parallel titrations.


We recommend using a sample of known concentration as a positive control. The concentration of the positive control sample should be within the linear section of the standard curve to obtain valid and accurate results.

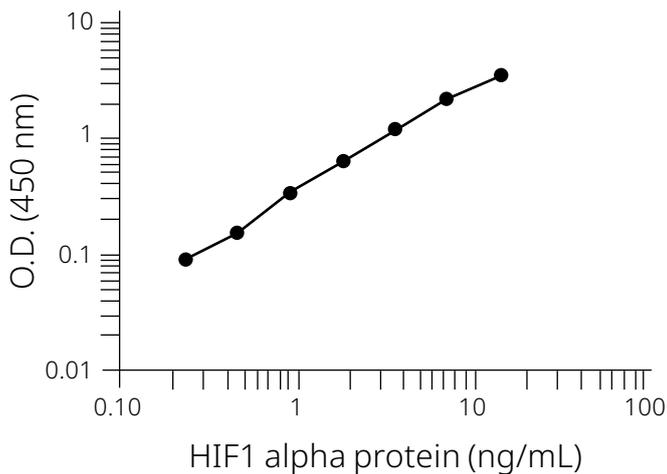


### Concentration of target protein in the sample

To determine the concentration of target protein concentration in each sample, first find the mean absorbance value of the sample. From the Y axis of the standard curve graph, extend a horizontal line from this absorbance value to the standard curve.

For example, if the absorbance reading is 1, extend the line from this absorbance point on the Y axis (a):

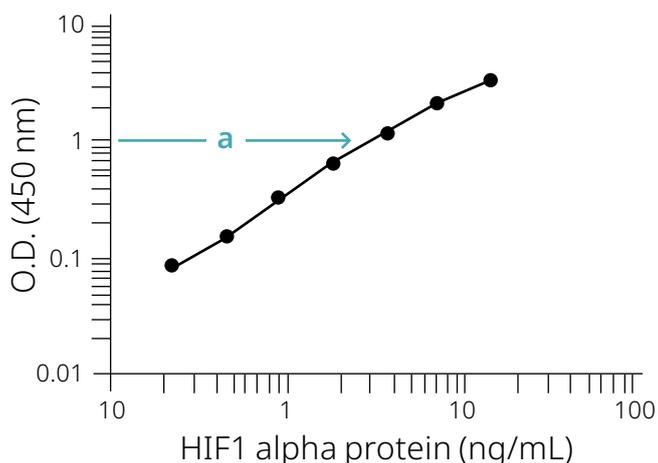

At the point of intersection, extend a vertical line to the X axis and read the corresponding concentration (b).

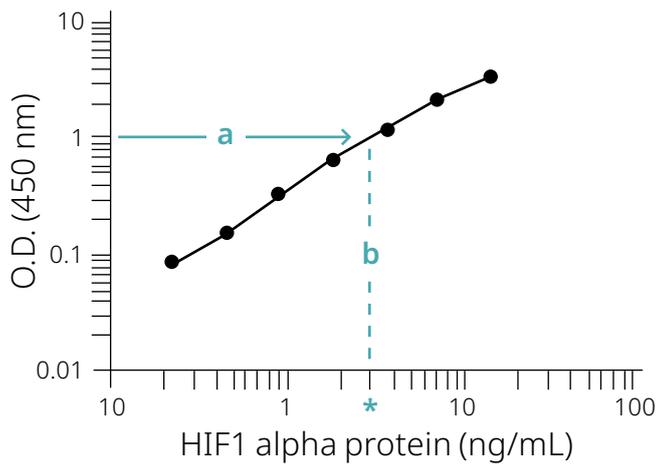

### **Samples that have an absorbance value falling out of the range of the standard curve**

To obtain an accurate result, these samples should be diluted before proceeding with the ELISA staining. For these samples, the concentration obtained from the standard curve when analyzing the results must be multiplied by the dilution factor.

### **Calculating the coefficient of variation**

The coefficient variation (CV) is the ratio of the standard deviation  $\sigma$  to the mean  $\mu$ :

$$C_v = \frac{\sigma}{\mu}$$

This is expressed as a percentage of variance to the mean and indicates any inconsistencies and inaccuracies in the results. Larger variance indicates greater inconsistency and error. Some computer programs can calculate the CV values from ELISA results.

#### **High CV can be caused by**

- Inaccurate pipetting; ensure pipette tips are sealed to the pipette before use so they draw up to correct volume of liquid
- Splashing of reagents between wells
- Bacterial or fungal contamination of either screen samples or reagents
- Cross contamination between reagents
- Temperature variations across the plate; ensure the plates are incubated in a stable temperature environment away from drafts
- Some of the wells drying out; ensure the plates are always covered at incubation steps

## **Spike recovery**

Spike recovery determines the effect sample constituents have on detection of the antigen by the antibody. For example, the many proteins contained in tissue culture supernatant may hinder antibody binding and increase the signal to noise ratio. This may result in underestimation of the target concentration.

Known concentrations of protein are spiked into both the sample matrix and a standard diluent. The spiked protein is quantified using the assay, and the results from the sample matrix and the standard diluent are compared.

If the results are identical, then the sample matrix is considered to be valid for the assay procedure. If the recovery is different, then components in the sample matrix are interfering with the analyte detection.

### **What if a spike recovery experiment indicated that the sample matrix is affecting the results?**

We recommend producing the standard curve using standard diluted in the sample matrix. Any effects on the results from the sample matrix will also be present in the standard, and therefore comparison between the standard curve and the samples is more accurate. Many of our ELISA kits contain a standard serum diluent for this purpose.

Another solution is to alter the sample matrix. For example, if neat biological sample is used, try diluting this in standard diluent. However, with this option, you will need to ensure that the dilution factor is taken into account when analyzing the results and that the concentration stays within the linear section of the standard curve.

# ELISA troubleshooting tips

## Poor standard curve

Cause	Solution
Improper standard solution	Confirm dilutions are made correctly.
Standard improperly reconstituted	Briefly spin vial before opening; inspect for undissolved material after reconstituting.
Standard degraded	Store and handle standard as recommended.
Curve doesn't fit scale	Try plotting using different scales, eg log-log, 5 parameter logistic curve fit.
Pipetting error	Use calibrated pipettes and proper pipetting technique.

## No signal

Cause	Solution
Incubation time too short	Incubate samples overnight at 4°C or follow the manufacturer guidelines.
Target present below detection limits of assay	Decrease dilution factor or concentrate samples.
Incompatible sample type	Detection may be reduced or absent in untested sample types. Include a sample that the assay is known to detect a positive control.
Recognition of epitope impeded by adsorption to plate	To enhance detection of a peptide by direct or indirect ELISA, conjugate peptide to a large carrier protein before coating onto the microtiter plate.
Assay buffer compatibility	Ensure assay buffer is compatible with target of interest (eg enzymatic activity retained, protein interactions retained).
Not enough detection reagent	Increase concentration or amount of detection reagent, following manufacturer guidelines.
Sample prepared incorrectly	Ensure proper sample preparation/dilution. Samples may be incompatible with microtiter plate assay format.
Insufficient antibody	Try different concentrations/dilutions of antibody.

<b>Cause</b>	<b>Solution</b>
Incubation temperature too low	Ensure the incubations are carried out at the correct temperature. All reagents including plate should be at room temperature or as recommended by the manufacturer before proceeding.
Incorrect wavelength	Verify the wavelength and read plate again.
Plate washings too vigorous	Check and ensure correct pressure in the automatic wash system. Pipette wash buffer gently if washes are done manually.
Wells dried out	Do not allow wells to become dry once the assay has started. Cover the plate using sealing film or tape for all incubations.
Slow color development of enzymatic reaction	Prepare substrate solution immediately before use. Ensure the stock solution has not expired and is not contaminated. Allow longer incubation.

### **Large coefficient of variation (CV)**

<b>Cause</b>	<b>Solution</b>
Bubbles in wells	Ensure no bubbles are present prior to reading plate.
Wells not washed equally/thoroughly	Check that all ports of the plate washer are unobstructed. Wash wells as recommended.
Incomplete reagent mixing	Ensure all reagents are mixed thoroughly.
Inconsistent pipetting	Use calibrated pipettes and proper technique to ensure accurate pipetting.
Edge effects	Ensure the plate and all reagents are at room temperature.
Inconsistent sample preparation or storage	Ensure consistent sample preparation and optimal sample storage conditions (eg minimize freeze/thaw cycles).

## High background

Cause	Solution
Wells are insufficiently washed	Wash wells as per protocol recommendations.
Contaminated wash buffer	Prepare fresh wash buffer.
Too much detection reagent	Ensure the reagent has been diluted properly or decrease the recommended concentration of detection reagent.
Blocking buffer ineffective (eg detection reagent binds blocker; wells not completely blocked)	Try different blocking reagent and/or add blocking reagent to wash buffer.
Salt concentration of incubation/wash buffers	Increasing salt concentrations may reduce non-specific and/or weak off-target interactions.
Waiting too long to read plate after adding stop solution	Read plate immediately after adding stop solution.
Non-specific binding of antibody	Use suitable blocking buffers, eg BSA or 5-10% normal serum - species same as primary antibody if using a directly conjugated detection antibody or same as secondary if using conjugated secondary. Ensure wells are pre-processed to prevent non-specific attachment.
High antibody concentration	Try different dilutions for optimal results.
Substrate incubation carried out in light	Substrate incubations should be carried out in the dark or as recommended by manufacturer.
Precipitate formed in wells upon substrate addition	Increase dilution factor of sample or decrease concentration of substrate.
Dirty plate	Clean the plate bottom.

## Low sensitivity

Cause	Solution
Improper storage of ELISA kit	Store all reagents as recommended. Please note that all reagents may not have identical storage requirements.
Not enough target	Concentrate sample or reduce sample dilution.
Inactive detection reagent	Ensure reporter enzyme/fluorophore has the expected activity.
Plate reader settings incorrect	Ensure plate reader is set to read the correct absorbance wavelength or excitation/emission wavelengths for fluorescent detection.
Assay format not sensitive enough	Switch to a more sensitive detection system (eg colorimetric to chemiluminescence/fluorescence). Switch to a more sensitive assay type (eg direct ELISA to sandwich ELISA). Lengthen incubation times or increase temperature.
Target poorly adsorbs to microtiter plate	Covalently link target to microtiter plate.
Not enough substrate	Add more substrate.
Incompatible sample type (eg serum vs cell extract)	Detection may be reduced or absent in untested sample types. Include a sample that the assay is known to detect as a positive control.
Interfering buffers or sample ingredients	Check reagents for any interfering chemicals. For example, sodium azide in antibodies inhibit HRP enzyme and EDTA used as anticoagulant for plasma collection inhibits enzymatic reactions.
Mixing or substituting reagents from different kits	Avoid mixing components from different kits.

## Matrix effect

ELISA quantification of plasma and serum occasionally encounters problems, which are caused by the matrix effect. The matrix effect can arise from a number of matrix components including, but not limited to: interaction between endogenous biological components, such as phospholipids, carbohydrates and endogenous metabolites (bilirubin), or an interaction between the analyte of interest and the matrix, such as covalent binding to plasma proteins. This results in erroneous sample readings.

Simply diluting the samples by 2–5 fold reduces the matrix effect; when diluting the samples, remember to use the same diluent as used for standard curve.

